

Optical Isolated Voltage Probe

(Powered by Battery)

OPB6015 (2.5V~5000V/150MHz)

OPB6025 (2.5V~5000V/250MHz)

OPB6035 (2.5V~5000V/350MHz)

OPB6050 (2.5V~5000V/500MHz)

OPB6080 (2.5V~5000V/800MHz)

OPB6100 (2.5V~5000V/1GHz)



产品说明书

Product User Manual

Preface

First of all, thank you for purchasing our products, this instruction manual is the description about the function, usage, operation attention points, etc. Before use, please read the instructions carefully and use correctly.

Manual annotation will use the following symbols to distinguish.



This symbol means it is harmful to the machine and human body; you must strictly follow the instruction manual to operate.

Warning

In the case of wrong operation, the user risk injury. The content under this mark records the relevant matters needing attention to avoid such dangers.

Notice

The user may suffer minor injuries and material damage with the wrong operation. To avoid such situation, the matters under this mark need attention.

Note

This symbolizes important note about how to use the machine.

To the safely use the machine, you must abide by the following safety precautions strictly.

The violation against the manual is likely to damage the protective function of the machine.

In addition, the company is not responsible for any safety problem caused by the violation of matters needing attention in operation.



- Please be careful to the danger of electric shock and pay attention to highest input voltage.
- Do not operate in wet or combustible conditions.
- Make sure the circuit under test is turned off before access it to the probe.
- Turn off the circuit after the measurement, and then remove the probe.
- When BNC cables are connected to the oscilloscope or other devices, ensure the BNC terminal is well grounded.
- Check the probe skin and probe lead regularly. If there is any breakage, stop using it immediately.

1. Introduction

OPB6000 series is the latest optical isolated voltage probe with remarkably high CMRR. The CMRR of traditional differential probe decreases fast in high-frequency range, as a result, measuring the small voltage signal waveform (e.g., the driving voltage when measuring the upper MOSFET of the half-bridge circuit) under high CM interference voltage accurately become a extremely hard task. OPB6000 series applies optical isolation technologies and gains remarkably high CMRR in all working bandwidth, helping our customers to deal with these kinds of challenging measurement with low cost.

Product Characteristics:

- 2 Chargeable batteries that can be replaced to keep the probe work continuously.
- Can be calibrated and zeroed online without disconnecting from the tested equipment.
- Automatic sleep function at the transmitting end (automatically wakes up when the receiving end is powered on; automatically sleeps 5 seconds after the receiving end is powered off)
- Multiple attenuators available, able to meet the measurement requirement of different voltage.
- Extremely high CMRR
- Isolation voltage over 60kV
- High accuracy and stability in wide temperature range
- Smaller size

2. Application

OPB6000 series can be widely applied in the R&D, debugging or maintenance of switching power supply, motor driver, new energy inverter, converter, LED power supply, household appliances and other electrical power devices.

- ☞ Floating signal test.
- ☞ Measure the gate voltage drive of power devices like Si/SiC/GaN .
- ☞ Small signal measurement of differential mode under high common mode voltage.

3. Electric Specification

Model	OPB6015	OPB6025	OPB6035	OPB6050	OPB6080	OPB6100
Bandwidth (-3dB)	150MHz	250MHz	350MHz	500MHz	800MHz	1GHz
Terminal load	1MΩ	1MΩ	1MΩ	50Ω	50Ω	50Ω
Output voltage range	±1.25V	±1.25V	±1.25V	±0.5V	±0.5V	±0.5V
Typical values of host noise (Vrms)	2mV	2mV	2mV	1mV	1mV	1mV
DC accuracy	≤±1%					
Isolation voltage (DC+Peak AC)	±60kV					
Standard configuration attenuator + host delay	15.3 ns (2-meter optical fiber)					
Battery specifications	Capacity				7.4V/950mA	
	Operating Time				About 8h	
	Standby time				About 30 days	
Power supply method	Rear end: USB 5V (P≥10W)					
Auto calibration	Yes					
operating temperature	-10℃-60℃					

Attenuator specifications

Probe Model	Attenuator Model	Connector type	Attenuation ratio	Measurement range	Maximum undamaged voltage	Input impedance
OPB6015 OPB6025 OPB6035	CK-AT2X-1-SMA	MMCX	2:1	$\pm 2.5\text{Vpk}$	2kVpp	$1\text{M}\Omega \parallel 28\text{pF}$
	CK-AT5X-1-SMA	MMCX	5:1	$\pm 6.25\text{Vpk}$	2kVpp	$0.93\text{M}\Omega \parallel 6\text{pF}$
	CK-AT10X-1-SMA	MMCX	10:1	$\pm 12.5\text{Vpk}$	2kVpp	$10.85\text{M}\Omega \parallel 6\text{pF}$
	CK-AT20X-1-SMA	MMCX	20:1	$\pm 25\text{Vpk}$	2kVpp	$10.40\text{M}\Omega \parallel 4\text{pF}$
	CK-AT50X-1-SMA	MMCX	50:1	$\pm 62.5\text{Vpk}$	3kVpp	$10.14\text{M}\Omega \parallel 2\text{pF}$
	CK-AT100X-1-SMA	MMCX	100:1	$\pm 125\text{Vpk}$	3kVpp	$10.06\text{M}\Omega \parallel 2\text{pF}$
	CK-AT200X-1-SMA	HVMCX	200:1	$\pm 250\text{Vpk}$	5kVpp	$9.94\text{M}\Omega \parallel 2\text{pF}$
	CK-AT500X-1-SMA	HVMCX	500:1	$\pm 625\text{Vpk}$	5kVpp	$20.43\text{M}\Omega \parallel 2\text{pF}$
	CK-AT1000X-1-SMA	HVMCX	1000:1	$\pm 1250\text{Vpk}$	6kVpp	$20.42\text{M}\Omega \parallel 2\text{pF}$
	CK-AT2000X-1-SMA	HVMCX	2000:1	$\pm 2500\text{Vpk}$	6kVpp	$42.02\text{M}\Omega \parallel 2\text{pF}$
	CK-AT4000X-1-SMA	5.08mm socket	4000:1	$\pm 5000\text{Vpk}$	12kVpp	$42.01\text{M}\Omega \parallel 2\text{pF}$
OPB6050 OPB6080 OPB6100	CK-AT5X-2-SMA	MMCX	5:1	$\pm 2.5\text{Vpk}$	2kVpp	$1\text{M}\Omega \parallel 28\text{pF}$
	CK-AT10X-2-SMA	MMCX	10:1	$\pm 5\text{Vpk}$	2kVpp	$0.97\text{M}\Omega \parallel 6\text{pF}$
	CK-AT20X-2-SMA	MMCX	20:1	$\pm 10\text{Vpk}$	2kVpp	$5.33\text{M}\Omega \parallel 6\text{pF}$
	CK-AT50X-2-SMA	MMCX	50:1	$\pm 25\text{Vpk}$	2kVpp	$10.40\text{M}\Omega \parallel 4\text{pF}$
	CK-AT100X-2-SMA	MMCX	100:1	$\pm 50\text{Vpk}$	3kVpp	$10.18\text{M}\Omega \parallel 2\text{pF}$
	CK-AT200X-2-SMA	MMCX	200:1	$\pm 100\text{Vpk}$	3kVpp	$10.08\text{M}\Omega \parallel 2\text{pF}$
	CK-AT500X-2-SMA	HVMCX	500:1	$\pm 250\text{Vpk}$	5kVpp	$9.94\text{M}\Omega \parallel 2\text{pF}$
	CK-AT1000X-2-SMA	HVMCX	1000:1	$\pm 500\text{Vpk}$	5kVpp	$20.44\text{M}\Omega \parallel 2\text{pF}$
	CK-AT2000X-2-SMA	HVMCX	2000:1	$\pm 1000\text{Vpk}$	6kVpp	$20.42\text{M}\Omega \parallel 2\text{pF}$
	CK-AT5000X-2-SMA	HVMCX	5000:1	$\pm 2500\text{Vpk}$	6kVpp	$42.02\text{M}\Omega \parallel 2\text{pF}$
	CK-AT10000X-2-SMA	5.08mm socket	10000:1	$\pm 5000\text{Vpk}$	12kVpp	$42.01\text{M}\Omega \parallel 2\text{pF}$


PS: 1. When the rise time of the measured signal is less than 3.5ns, the oscilloscope's impedance should be set to 50Ω to ensure accurate measurement.
2. Attenuators with MMCX connector type can be paired with SSMB-type connectors.
3. OPB6015/OPB6025/OPB6035 with standard CK-AT20X-1-SMA; OPB6050/OPB6080/OPB6100 with standard CK-AT50X-2-SMA.; If you need other attenuator, please purchase independently.
The maximum test voltage decreases as the test frequency increases, as shown in the table below.

Maximum test voltage	Maximum test frequency
$\pm 5000\text{Vpk}/\pm 2500\text{Vpk}$	700kHz/800kHz
$\pm 1000\text{Vpk}/\pm 500\text{Vpk}$	2MHz/3MHz
$\pm 250\text{Vpk}/\pm 100\text{Vpk}$	20MHz/50MHz
$\pm 50\text{Vpk}/\pm 25\text{Vpk}$	100MHz/200MHz


Optional attenuator packing list

Connector type	MMCX	HVMCX	5.08mm socket
CK-24 (HVMCX-KE)	—	3	—
CK-202 (5.08_2p)	—	—	5
CK-326 (HVMCX/RG316)	—	1	—

Common mode rejection ratio curve of different attenuators

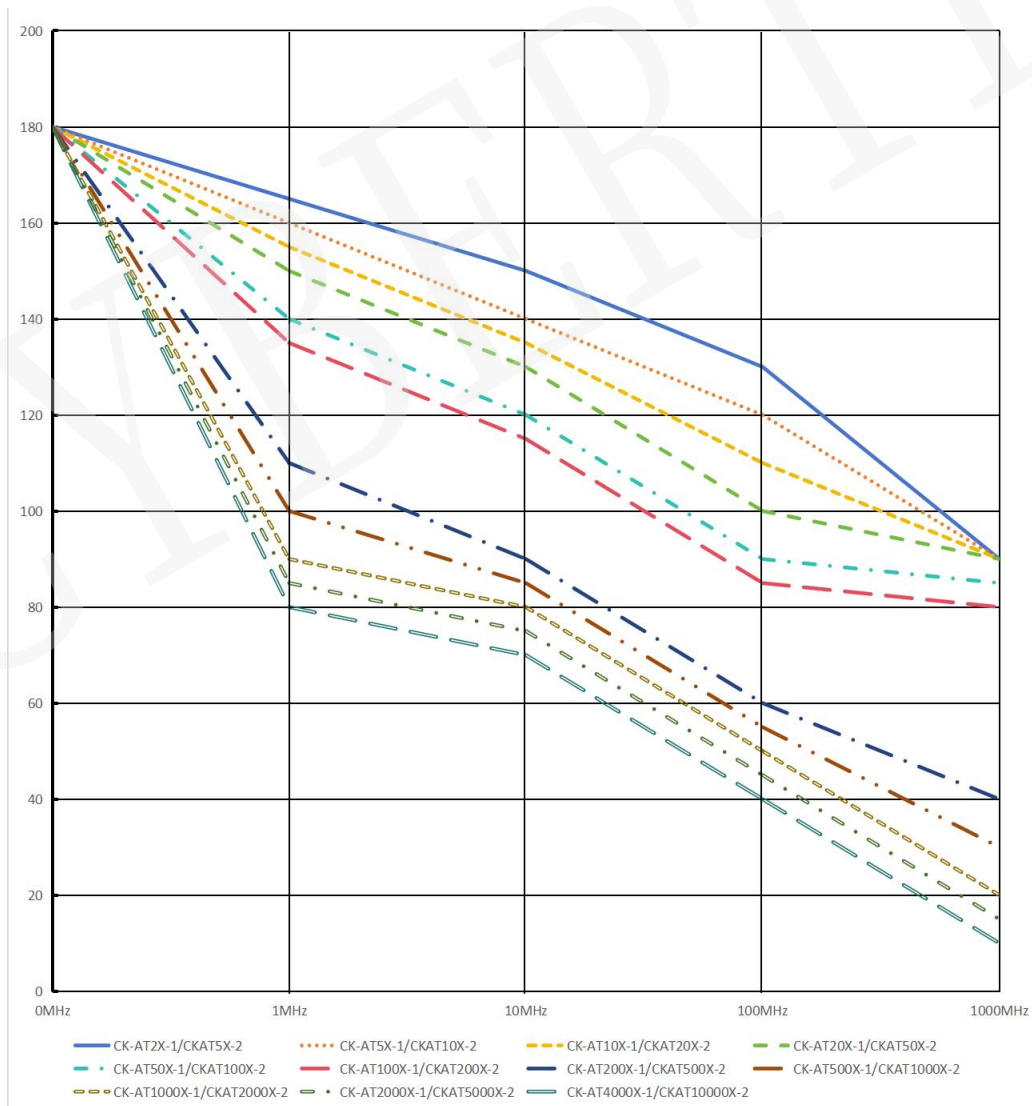


4. Probe instruction

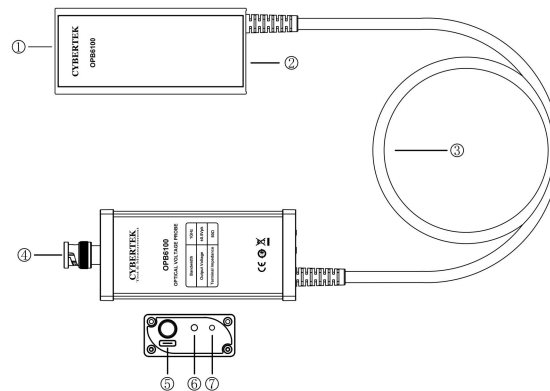


- ① Attenuator input connector:SMA socket.
- ② Power supply indicator light: green light means sufficient power, red light means low power.
- ③ Optical fiber: do not press it heavily or bend it to 90 degrees, or the fiber will be broken.
- ④ Output connector: standard BNC output connector.
- ⑤ Power supply connector: please use adaptor and power supply cable of 5V. This device may not work properly with insufficient power supply.
- ⑥ Dual color indicator light: the green light blinking means the auto-zero set is ongoing, and if there's three beeps and the green light remains, the adjustment is successfully done. However if the buzzer sound continuously for 1~2 sec with the green light on, the auto-zero setting is failed. If the red light is on, the probe is malfunctioned, you would probably need to send it back for maintenance.
- ⑦ Auto-zero set button: press it lightly to activate the auto-zero set function.

Battery Removal & Installation Guide


Step 1:

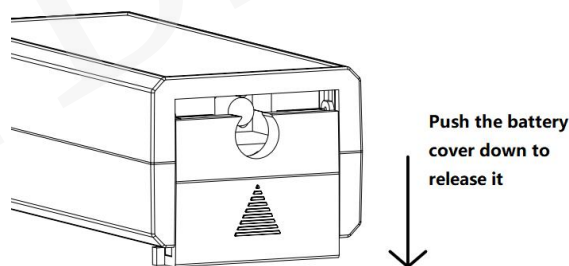

Step 2:

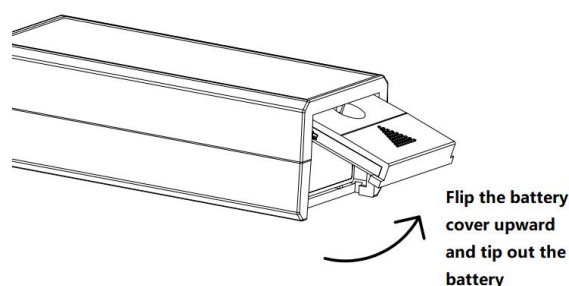

Main Accessories Diagram:

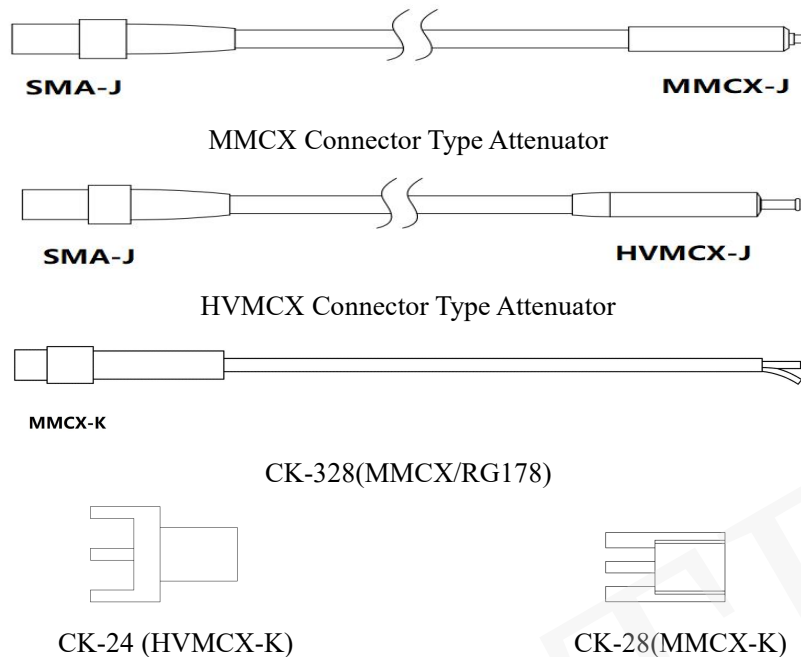

NOTE

- Do not put heavy object (for instance, your chair) on the optical fiber, avoiding stress on the fiber is crucial to avoid malfunction.
- Do not squeeze, curl, or bend the optical fiber violently. The diameter of bending should be over 10cm.
- Do not twist or tie the optical fiber. Do not pull or jerk the optical fiber, especially when there are twists or knots.
- Do not drop the probe, this could damage the inner optical component.
- Please store the probe in our standard case as we did when you don't need to use it.
- Please careful exam the optical fiber before usage, and if there's anything broken, please stop using it at once.

5. Operating Process

Attention

Please use our standard adaptor and power supply cable.

- Estimate the range of voltage under test and insert the proper attenuator.
- Connect the probe to the oscilloscope and power it up. Activate the auto-zero set, it will take about 20 sec depends on the environmental temperature and main component temperature.If calibration fails, you can power off and restart.
- Set up the attenuation ratio of the oscilloscope accordingly, and adjust the sensitivity of the oscilloscope according to the voltage under test.
- Make sure the front end of the probe is elevated if possible, keeping it away from the high voltage pulse circuit can decrease the interference on the probe.
- The front end of the probe is directly connected with the high voltage circuit under test. Do not take the probe off before you turn off the circuit's power supply.

6. Mechanical Specifications

Model		Parameter
Probe dimensions	Front-end E/O transmitter	Around 102*45*33mm
	Rear-end O/E receiver	Around 106*49*23mm
Attenuator length		Around 200mm
Optical fiber length		2m
Probe Weight		Around 400g

7. Warranty

Please refer to the instruction on the warranty card.

8. Packing list

Name	OPB6015	OPB6025	OPB6035	OPB6050	OPB6080	OPB6100
Voltage Probe	1	1	1	1	1	1
20X attenuator (CK-AT20X-1-SMA)	1	1	1	-	-	-
50X attenuator (CK-AT50X-2-SMA)	-	-	-	1	1	1
MMCX female socket to DuPont cable connector (CK-327)	2	2	2	2	2	2
MMCX female socket (CK-28)	5	5	5	5	5	5
USB power supply cable TYPE-C (CK-314A)	1	1	1	1	1	1
Power supply adaptor 5V(CK-605)	2	2	2	2	2	2
OE transmitter support frame (CK-690B)	1	1	1	1	1	1
Input extension cable (CK-328)	2	2	2	2	2	2
Output extension cable(CK-325)	1	1	1	1	1	1
Battery charger set (CK-691)	1	1	1	1	1	1
Instruction manual	1	1	1	1	1	1
Warranty card	1	1	1	1	1	1
Test report	1	1	1	1	1	1

CYBERTEK

SHENZHEN ZHIYONG ELECTRONICS CO., LTD.

Addr: Room A1702, Building 4, TianAn Cyber Park, HuangGe Road, LongGang
District, ShenZhen City, China

Tel: (86) 400 852 0005 / (86 755) 86628000

Q Q: 400 852 0005

Email: cybertek@cybertek.cn

Url: <http://www.cybertek.cn>

© Zhiyong Electronics, 2026

Published in China, Jul. 01, 2026